



CryOmega®

Disposable Cryosurgical Device

Clinically effective direct
application of liquid
nitrous oxide (-89°C/-127°F).

In a convenient and
economical device!



NEW

Watch Online Video Tutorials by Visiting
www.YouTube.com/PremierMedProducts



Premier® Medical Products
www.premusa.com

It's as easy as



CryOmega® - Disposable cryosurgical unit containing 16g nitrous oxide (N₂O) cartridge.

Effective

Continuous direct spray of liquid nitrous oxide (-89°C/-127°F) produces clinically effective freezing versus canister-based systems. Pinpoint precision prevents destruction of healthy tissue.

Convenient

Activate internal cartridge once and the device is ready for use. No time wasted on pre-procedure tip saturation, filling of cryogen reservoirs, etc. No additional accessories or cartridges needed. Simply aim and spray!

Economical

Each unit has 4 minutes (240 seconds) of total spray time and can be used for multiple procedures. Recommended spray times for treating each of the FDA-cleared lesions are provided below.

Disposable


Simply dispose of the entire unit with normal medical waste when the internal nitrous oxide cartridge is empty.

CryOmega®		Treatment Spray Times (seconds by approved lesion)			
Verruca Vulgaris	10 – 20		Actinic Keratosis	5	
Verruca Plantaris	10 – 20		Lentigo	2 - 5	
Verruca Plana	5 – 15		Molluscum Contagiosum	3 - 10	
Skin Tags	5 – 10		Genital Lesions	5 - 12	
Seborrheic Keratosis	5 – 10		Total Cartridge Spray Time	4 minutes (240 seconds)	

Cryosurgery is contra-indicated in patients with cryoglobulinemia. Please refer to Product Insert for relative contraindications and general precautions when using CryOmega.

Achieving low temperatures is the key to clinically effective and successful cryosurgical application!

By delivering a continuous direct spray of nitrous oxide, CryOmega consistently produces the temperatures required to successfully treat warts, skin tags and other common benign skin lesions in any clinical setting.

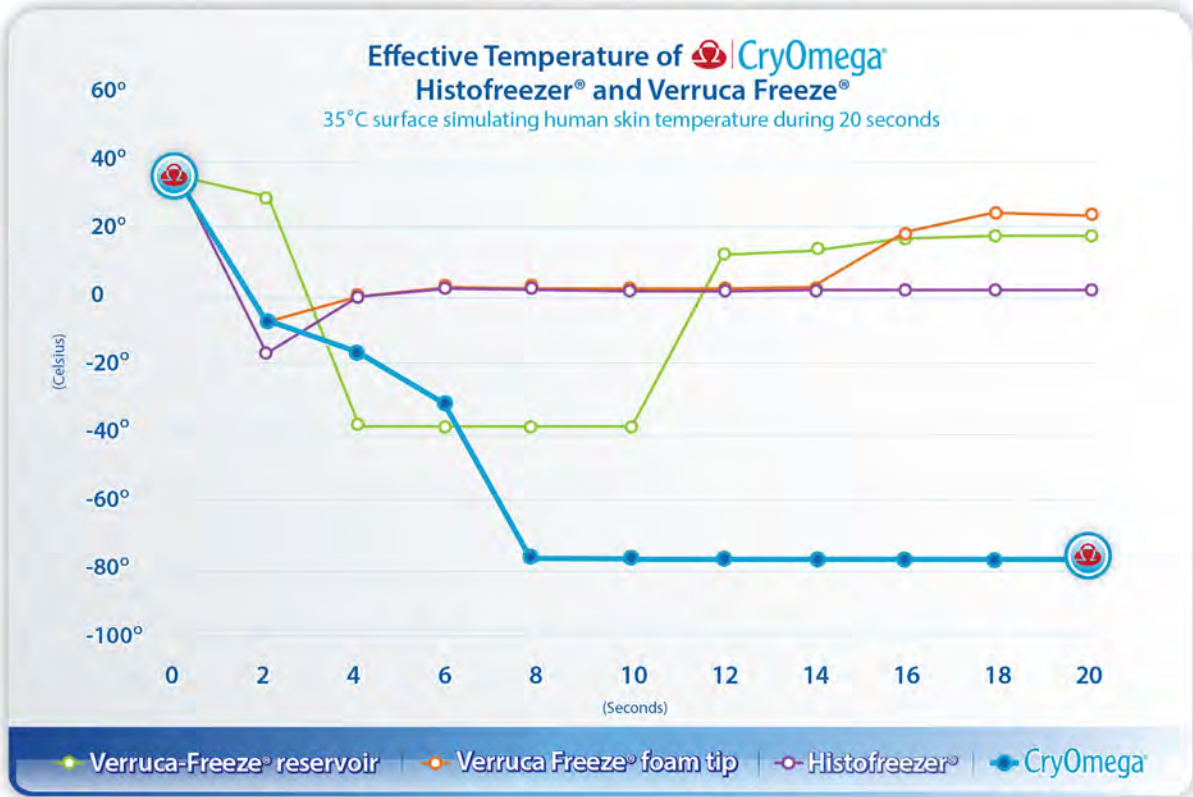

* Data on file



Technique Tip:

During some procedures there may be a build-up of frost when using CryOmega. This frost can act as an insulator and prove beneficial in helping to maintain the desired temperature of the tissue. Room temperature and humidity, along with spray time, spray distance and spraying motion, play a role in frost build-up. Spray time is determined by the type and size of lesion treated. Recommended spray distance is approximately 1 cm and should be applied in small circular motions.

Instructional online video tutorials featuring CryOmega are available on YouTube and can be found by searching keywords "Premier CryOmega" or "Premier Medical Products". You may also access our channel directly by visiting, www.YouTube.com/PremierMedProducts

CryOmega®

Disposable Cryosurgical Device

“ I believe the CryOmega® device is appropriate for all Primary Care Physicians. It's a great way to introduce cryosurgery for physicians who don't realize how important full-time cryosurgery is for their practice. ”

John E. Hocutt, Jr. M.D., FAAFP

Ordering Information

9034000 CryOmega®

Disposable cryosurgical unit containing 16gm nitrous oxide (N₂O) cartridge.



Single Unit

9034002 CryOmega® Twin Pack

Contains 2 CryOmega units, each containing a 16gm nitrous oxide (N₂O) cartridge for your convenience.



Twin Pack

Contact Premier® Medical Products for more information.

CryOmega is available through your medical or surgical supply distributor.

Available from:



Premier® Medical Products

1710 Romano Drive, Plymouth Meeting, PA 19462 U.S.A.
610-239-6053 • 888 PREM USA (773-6872) • Fax: 610-239-6171
cryomega@premusa.com • www.premusa.com